

1

Introduction

1.1 Atomic Optical Emission Spectrochemistry (OES)

1.1.1 Conventional OES

Since the early 1800s, scientists realized that elements emitted specific colors of light. As atomic theory developed, spectroscopists learned that those colors, wavelengths, or frequencies were a unique signature for each atom and ion. Hence spectra became the fingerprints of the emitting atomic species. This is the basis for atomic spectrochemical analysis.

Early sources of spectra were the sun, flames, and gas discharges, such as the old Geissler tube. These were plasma sources, with varying degrees of ionization depending on the source conditions. Against the 5000 K photosphere of the sun, we see the Fraunhofer absorption lines due to neutral and once ionized species. In the solar corona, highly ionized spectra are observed because of plasma temperatures that reach into the hundreds of thousands of degrees.

Many sources have been developed for spectrochemistry, but two workhorses have been the conventional electrode spark and, more recently, the inductively coupled plasma (ICP). These are illustrated in Figure 1.1, which also contains a photograph of the laser spark. The electrode spark has excitation temperatures of up to 50 000 K, while the argon ICP temperature is more typically about 10 000 K. Usually these sources are used for laboratory analyses, but occasionally they are pressed into service for situations requiring more rapid data acquisition. For example, the conventional spark has been used for decades to monitor the steel-making process by withdrawing a molten sample that is then solidified and transported to a laboratory located in the plant for rapid analysis. Decisions on additives are made based on the resulting spectroscopic data.

1.1.2 Laser OES

As soon as the laser was developed in the early 1960s, spectrochemists began investigating its potential uses (Radziemski, 2002). An early observation was that a pulsed laser

2 Handbook of Laser-Induced Breakdown Spectroscopy

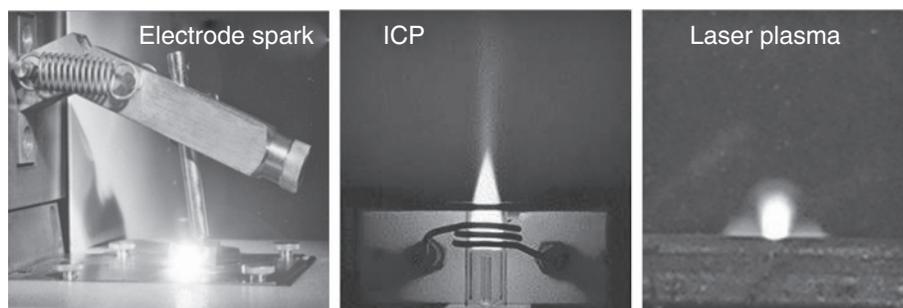


Figure 1.1 Photographs of a conventional spark, an inductively coupled plasma (ICP), and a laser-induced spark formed on a metal showing blue emission (color plate) due to AlO molecules. The size scales are different. [Photos courtesy of: Westmoreland Mechanical Testing & Research, Inc. (spark) and Exova, Inc., Santa Fe Springs, CA Health Sciences Lab (ICP).] (For color details please see color plate section.)

could produce a small plasma in air and on metals (Figure 1.1). The emission from that plasma showed the potential for spectrochemical analysis. However, from 1960 to 1980, the analytical capability was inferior to that of the conventional spark and laser technology was in its infancy, so the technique was less favored than a related one—laser ablation into a conventional plasma source. Here the laser was used to vaporize a small amount of sample for analysis by, for example, the conventional electrode spark (Moenke and Moenke-Blankenburg, 1973). However, that was not the only way the laser could be used in spectrochemistry.

The development of tunable dye lasers meant that one could illuminate a prepared source of atoms with radiation resonant with a transition in one of the atomic species. Then either the absorption of the laser beam or the laser-induced fluorescence could be used as an analytical signal. These techniques discriminated against the background and increased the signal to noise considerably by recycling the same atoms many times. Sometimes the atoms were placed in the laser cavity itself. The intracavity absorption technique was a very sensitive spectrochemical method, if difficult to employ generally.

Both absorption and fluorescence are used in many applications. However, because the laser must be tuned to a specific transition in a specific species, it is not as broadly useful as a hot plasma in which a variety of species can be excited and monitored simultaneously.

1.2 Laser-Induced Breakdown Spectroscopy (LIBS)

Laser-induced breakdown spectroscopy (LIBS), also sometimes called laser-induced plasma spectroscopy (LIPS) or laser spark spectroscopy (LSS) has developed rapidly as an analytical technique over the past three decades. As most commonly used and shown schematically in Figure 1.2, the technique employs a low-energy pulsed laser (typically tens to hundreds of mJ per pulse) and a focusing lens to generate a plasma that vaporizes a small amount of a sample. A portion of the plasma light is collected and often directed to a spectrometer by a fiber optic. The spectrometer disperses the light emitted by excited atoms, ions, and simple molecules in the plasma, a detector records the emission signals,

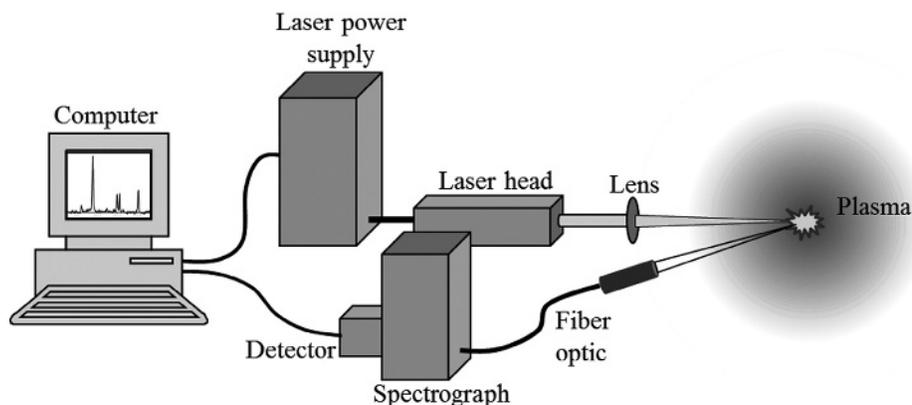


Figure 1.2 A schematic of a general apparatus for laser-induced breakdown spectroscopy illustrating the principal components.

and electronics take over to digitize and display the results. The book cover shows a LIBS spectrum with certain strong spectral features standing out from the continuous background plasma light.

LIBS is an appealing technique compared to many other types of elemental analysis, because setting up an apparatus to perform a LIBS measurement is very simple. One merely focuses a laser pulse in or on a sample, which can be a gas, liquid, aerosol, or solid, to form a microplasma, examples of which are shown in Figure 1.3.

The spectra emitted are used to determine the sample's elemental constituents. However, the basic physical and chemical processes involved are not so simple. The initiation, formation and decay of the laser plasma are complex processes. Absorption of the incident laser radiation occurs through the mechanism of inverse bremsstrahlung, involving three body collisions between photons, electrons, and atoms or molecules. In gases and liquids, the plasma creates a shock wave in the surrounding medium transferring energy by means of conduction, radiation, and the shock wave. When the experiment deals with a sample surface in a vacuum, the plasma and ejecta expand freely away from the surface at different speeds. Excitation of specific energy levels in different atoms is likewise complex, and depends on factors such as thermodynamic equilibrium and interactions with other atoms and molecules generally lumped under the category of matrix effects. After the laser pulse has terminated, the plasma decays over an interval of one to several microseconds, depending on the laser energy deposited. In vacuum, that temporal process is shortened. Most LIBS experiments involve repetitive plasmas at frequencies of 10 Hz or greater.

The spectra observed change as the plasma evolves temporally as shown in Figure 1.4. Soon after plasma initiation, continuum and ionic spectra are seen. The continuum is the “white light” from the plasma that contains little spectroscopic information and the ions result from electrons ejected by neutral atoms. As the plasma decays, these are followed by spectra from neutral atoms, and eventually simple molecules formed from the recombination of atoms. Throughout the temporal history, one observes a diminishing continuum spectral background due to recombination of free electrons with ions. Inspection of the LIBS spectrum reveals immediate qualitative information about sample composition.

4 Handbook of Laser-Induced Breakdown Spectroscopy

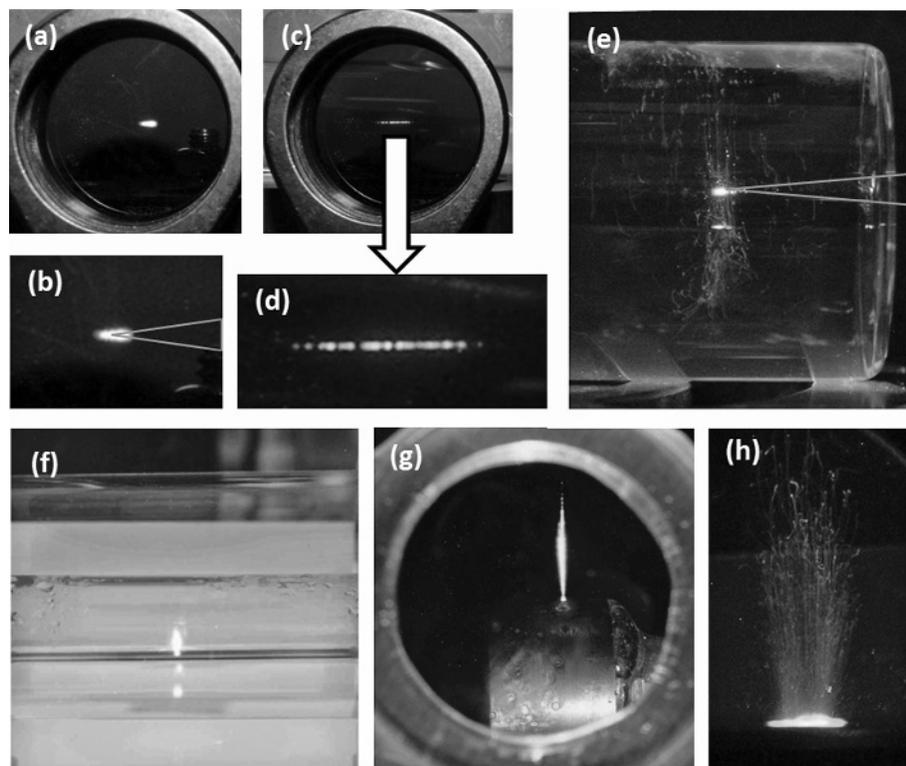


Figure 1.3 Laser sparks in different media: (a) in air; (b) expanded image of the air spark with incident laser pulse direction indicated; (c) spark in aerosol-laden air; (d) expanded image of (c); (e) in bulk liquid with incident laser pulse direction indicated (the streamers surrounding the spark are gases evolved from the focal region); (f) on a liquid surface; (g) on a beryllium metal piece; and (h) a long spark formed on aluminum metal by a cylindrical lens showing strong particle production. Photos (a) through (d) were taken through a neutral density filter. (For color details please see color plate section.)

After calibration, quantitative information can be obtained. These issues will be treated in greater depth in subsequent chapters.

During the past 20 years, the LIBS technique has made significant progress toward becoming a viable commercial technology. Through the year 2000, several useful reviews were published (Adrain and Watson, 1984; Cremers and Radziemski, 1987; Radziemski and Cremers, 1989; Radziemski, 1994; Lee *et al.*, 1997). Since then, the methods of disseminating LIBS information have expanded considerably, as will be discussed in Section 1.6.

In this chapter, we consider the history of the technique and some applications that have spurred its development. We focus on the first time an innovation or application appeared on the scene, rather than tracing every innovation through to the present day. Note, however, that contemporary improvements in apparatus, techniques, and fundamental understanding are driving re-examinations of old applications. Conversely, the emergence of new applications drives improvements in a recurring upward spiral of progress. Table 1.1

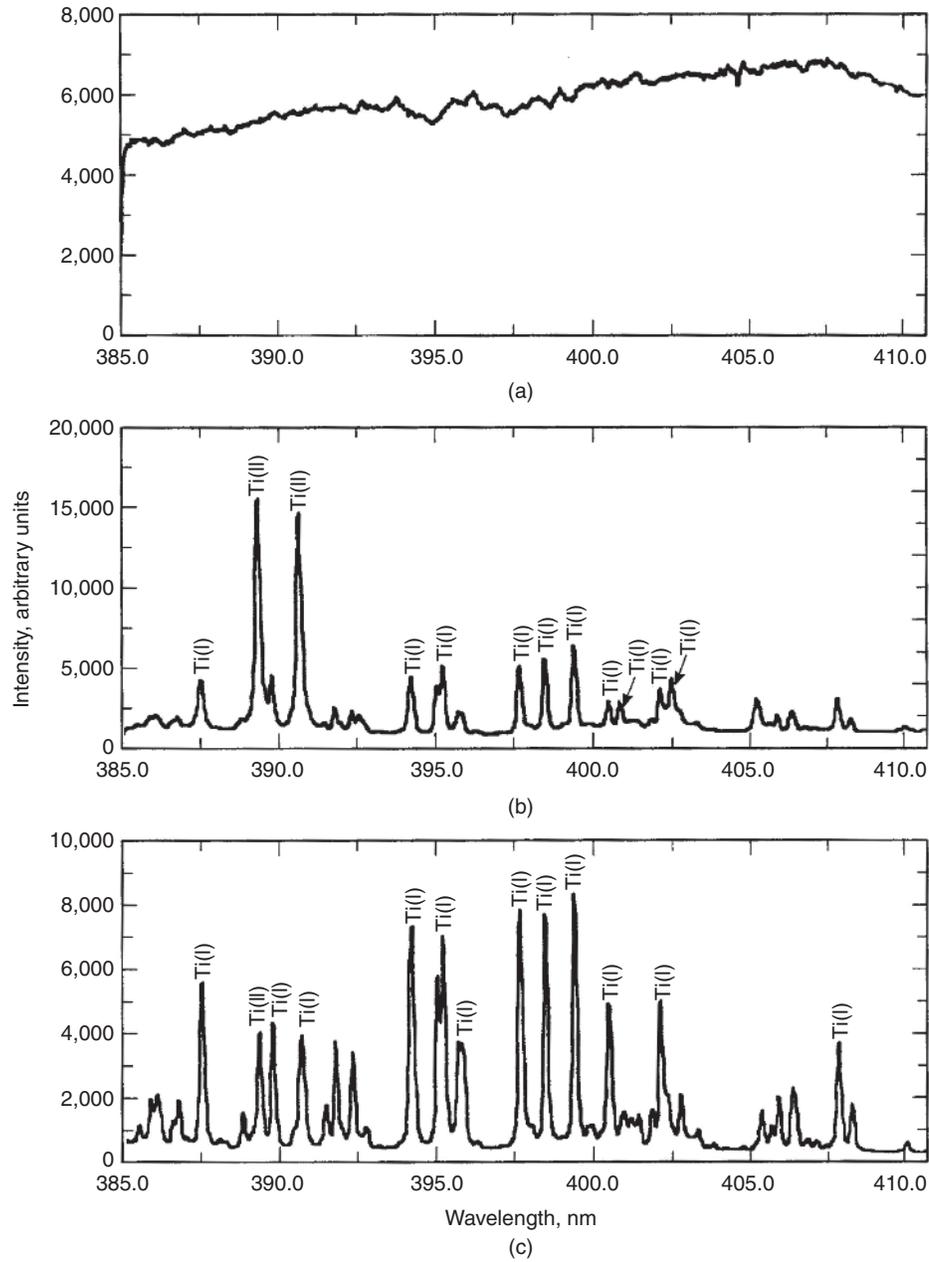


Figure 1.4 Gated titanium spectra of a LIBS plasma illustrating the development of the spectrum as a function of the time after plasma initiation. From top to bottom, the time intervals are (a) 0–0.5 μ s; (b) 0.5–5 μ s, and (c) 10–110 μ s.

6 *Handbook of Laser-Induced Breakdown Spectroscopy***Table 1.1** *Significant milestones in the development of laser-induced breakdown spectroscopy (LIBS) as an analytical technique applicable to a variety of samples and circumstances*

1960	Ted Maiman develops the first pulsed laser
1963	First analytical use of a laser plasma on surfaces, hence the birth of LIBS
1963	First report of a laser plasma in a gas
1963	Laser microspectral analysis demonstrated, primarily with cross-excitation
1963	Laser plasmas in liquids were initially investigated
1964	Time-resolved laser plasma spectroscopy introduced
1966	Characteristics of laser-induced air sparks studied
1966	Molten metal directly analyzed with the laser spark
1970	Continuous optical discharge (COD) reported
1970	Q-switched laser use reported, results compared with normal laser pulses
1971	Biological materials investigated with LIBS
1972	Steel analysis carried out with a Q-switched laser
1978	Laser spectrochemical analysis of aerosols reported
1980	LIBS used for corrosion diagnostics in nuclear reactors
1982	Initial use of the acoustic properties of the laser-induced spark
1984	Analysis of liquid samples and hazardous aerosols demonstrated
1988	Attempts made to enhance intensities through electric and magnetic fields
1989	Metals detected in soils using laser plasma method
1992	Portable LIBS unit for monitoring surface contaminants developed
1992	Stand-off LIBS for space applications demonstrated
1993	Underwater solid analysis via dual-pulse LIBS demonstrated
1994	Papers on statistical analysis of LIBS data began appearing
1995	Demonstration of fiber-optic delivery of laser pulses
1995	Multiple-pulse LIBS reported for use on steel samples
1997	LIBS used in applications in painted works of art and illuminated manuscripts
1998	Subsurface soil analysis by LIBS-based cone penetrometers shown
1998	Reports on the use of echelle spectrometers coupled with CCD detectors
1999	Trace metal accumulation in teeth observed with LIBS
1999	Pulses from different lasers used to enhance LIBS performance
1999	Calibration-free LIBS introduced
2000	Report on commercial instrument for coal analysis
2000	Demonstration of LIBS on a NASA Mars rover
2000	First International Conference on LIBS—Pisa, Italy
2002	Second International Conference on LIBS—Orlando, USA
2002	Detection of explosives, chemical, and biological threats increases in importance
2004	Third International Conference on LIBS—Malaga, Spain
2004	LIBS approved for 2011 Mars Science Laboratory Rover mission
2005	Increasing emphasis on molecular identification with LIBS or LIBS-Raman
2006	Fourth International Conference on LIBS—Montreal, Canada
2008	Fifth International Conference on LIBS—Berlin Aldershof, Germany
2010	Sixth International Conference on LIBS—Memphis, US
2011	Mars Science Lander mission launched with LIBS instrument on board
2012	LIBS instrument on Mars Science Laboratory Rover in operation
2012	Seventh International Conference on LIBS, Luxor, Egypt

illustrates some significant milestones in LIBS development. These will be addressed individually in the following sections.

1.3 LIBS History 1960–1980

Shortly after the pulsed ruby laser was invented in 1960, the laser-induced plasma was observed. The first published report mentioning the plasma was a meeting abstract by Brech and Cross (1962). Early on, the laser was used primarily as an ablation source with cross-excitation by an electrode spark to provide the spectrum. In 1963, Debras-Guédon and Liodec published the first analytical use for spectrochemical analysis of surfaces (Debras-Guédon and Liodec, 1963). Maker *et al.* (1964) reported the first observation of optically induced breakdown in a gas. Runge *et al.* (1964) in the same year discussed the use of a pulsed Q-switched ruby laser for direct spark excitation on metals. Linear calibration curves were obtained for nickel and chromium in iron, with precisions of 5.3% and 3.8%, respectively. They also analyzed molten metal. In 1966, Evtushenko looked at the effect of sparks from two lasers (Evtushenko *et al.*, 1966). About the same time, Young *et al.* (1966) described the characteristics of laser-induced air sparks.

In the period from 1964 to 1967, the first instruments based primarily on laser ablation with cross-excitation were developed by Zeiss (Germany), Jarrell-Ash (USA), and JEOL Ltd. (Japan). Although they could be operated with the laser plasma generating the spectral emissions, most often the laser was used only for ablation followed by cross-excitation with a conventional spark. Because the auxiliary spark could contaminate and complicate the analysis through the introduction of electrode material, auxiliary excitation by electrodeless methods was also developed. The instruments could not typically compete in accuracy and precision with conventional spark spectroscopy, although they could analyze nonconducting samples. Some instruments continued in use through the 1990s. An excellent discussion of those devices and the associated techniques is contained in the book entitled *Laser Micro Analysis* by Moenke-Blankenburg (1989).

Time resolution of the decaying plasma helps to monitor the plasma evolution, to discriminate against the continuum light, and to sort out spectral features. It is especially valuable in reducing interferences between spectral features that appear at the same or adjacent wavelengths but in different temporal windows as illustrated in Figure 1.4. Different detection systems to obtain temporally resolved spectra were used in the 1960s, including a streak camera and rotating mirrors. A method more suited to modern detectors, electronically gating and averaging the signals from many plasmas, was developed by Schroeder *et al.* (1971). As detectors have developed, the preferred methods of time resolution have moved from boxcar averagers, for example, to gated, intensified charge-coupled devices (ICCDs), to electron-multiplying CCDs (EMCCDs).

Fast photodetectors are used to record the temporal profile of plasma emissions from single pulses. An early review of the field was published by Scott and Strasheim (1970). Multiple-pulse LIBS was introduced by Piepmeier and Malmstadt (1969), and Scott and Strasheim (1970). In both cases the multiple pulses were generated from the same laser during the same extended flashlamp excitation by alternately frustrating and enabling Q-switched pulses.

8 Handbook of Laser-Induced Breakdown Spectroscopy

During this period, much of the research on the laser plasma and its uses appeared in the Russian literature. For example, Afanas'ev and Krokhin (1967) published on the vaporization of matter exposed to laser emission. Raizer (1966) reported on the breakdown and heating of gases under the influence of a laser beam, which was a summary of original work and a review of the state of the art. Biberman and Norman (1967) did a thorough analysis of the origins of the continuous spectrum from the laser plasma which underlies the discrete spectral lines. Buravlev *et al.* (1974) commented on using a laser for spectral analysis of metals and alloys. Much of the physics covered in the Russian literature was summarized in the classic book by Raizer, *Laser-Induced Discharge Phenomena*, published in English (Raizer, 1977). Underlying that is the classic book on the physics of shock waves and high-temperature hydrodynamic phenomena, a text originally published in Russian in 1964, translated into English in 1966, and recently reprinted by Dover books (Zel'dovich and Raizer, 2002).

Early on, it was recognized that physical and chemical matrix effects would have to be dealt with if LIBS was to develop as a quantitative method. Cerrai and Trucco (1968) discussed matrix effects in laser-sampled spectrochemical analysis. They focused on the dependence of spectral line intensities on physical conditions such as grain sizes and boundaries. This was followed by a 1971 paper by Marich *et al.* concluding that physical effects were more important than chemical ones. However others, like Scott and Strasheim (1970), found signal suppression due to various effects linked to the components of the matrix. It is now accepted that a variety of physical and chemical effects play important roles in signal strength and repeatability. Biological media with metallic contamination were investigated using the laser plasma as reported in papers by Marich *et al.* (1970) and Treytl *et al.* (1972). The former deals with the effect of the matrix on the spectral emission from a variety of samples, including human serum and liver. The latter provides detection limits for the analysis of metals in biological materials. Here, metals in the form of reagent grade salts were incorporated into gelatin or albumin matrices. Limits of detection ranged from 2×10^{-15} g for magnesium and copper to 3×10^{-13} g for mercury and iron.

A novel variation of the pulsed plasma is the continuous optical discharge (COD). In this case a CW laser beam is focused to sustain a plasma as long as the laser remains operating. The laser is usually of the continuous CO₂ variety. Initiation requires another pulsed laser or a conventional spark. Early papers on this subject were published by Generalov *et al.* (1970) and Keefer (1974). Spectrochemical analysis by the COD was investigated by Cremers *et al.* (1985).

Material processes such as welding were obvious applications of high-powered lasers. The plasma literature in that field overlapped with that of spectrochemical applications. In the first of a series of books, Ready (1971) provided an overview of the variety of phenomena induced by high-power laser pulses. Some of the subjects discussed were: optical damage of materials; the interaction between laser radiation and surfaces resulting in ablation, melting, and crater formation; the effect of laser light on biological systems; and optically induced gas breakdown. A more recent version edited by Ready is a compendium of 30 years of research, the *LIA Handbook of Laser Materials Processing* (Ready, 2001).

Generating a plasma in water was considered first by Buzukov *et al.* (1969). Lauterborn (1972) conducted high-speed photography of plasmas in liquids. This was followed by

measurements of shock waves and cavities caused by laser-induced breakdown in water, glycerin, and benzene by Teslenko (1977). These mechanistic studies focusing on the shock wave formation and propagation continued throughout the 1970s.

In the mid- to late-1970s, aerosols became a subject of research. The effects of dust and particles in the beam as they influenced breakdown were studied and reported by Lencioni (1973). He found that when long focal-length lenses were used, the dust in the beam initiated strings of mini-plasmas. Belyaev *et al.* (1978) discussed laser spectrochemical analysis of aerosols. In 1979, Edwards and Fleck published on the two-dimensional modeling of aerosol breakdown in air (Edwards and Fleck, 1979). This was followed by a study in 1982 by Ivanov and Kopytin on the selective interaction of a train of laser pulses with an aerosol medium (Ivanov and Kopytin, 1982).

A spin-off method of LIBS called TABLASER was described by Measures and Kwong in 1979 (Measures and Kwong, 1979). That technique uses an ablation laser pulse followed by a laser pulse through the plume. The second pulse from a dye laser is tuned to a transition in the element of interest and results in laser-induced fluorescence. Interest in this type of arrangement surfaced again in the 1990s.

1.4 LIBS History 1981–1990

As lasers and other LIBS components became smaller and the *in situ* advantages of the laser plasma became more obvious, additional applications appeared. Interest at Los Alamos National Laboratory was kindled by two 1981 papers on the time-integrated (Loree and Radziemski, 1981) and time-resolved (Radziemski and Loree, 1981) forms of the technique in gases. The term LIBS was originally used in the former 1981 paper, and TRELBS, identified with the time-resolved version, in the latter. Currently LIBS is the term used for either method.

Los Alamos then funded an internal study of the use of this technique for the detection of toxic beryllium dust, resulting in papers on detecting beryllium in air (Radziemski *et al.*, 1983a) and on filters (Cremers and Radziemski, 1985). Figure 1.5 shows a long spark created by using a cylindrical lens, on a rotating stage on which a blackened piece of filter paper has been set for contrast. During that period, Los Alamos scientists studied the detection of hazardous gases (Cremers and Radziemski, 1983), aerosols (Radziemski *et al.*, 1983b), and liquids (Cremers *et al.*, 1984; Wachter and Cremers, 1987). Sensing of steels and other metals in molten or solid forms were also investigated along with the beginnings of LIBS for stand-off analysis (Cremers, 1987). Beginning in 1989, the use of LIBS for determining metals (Cr and Pb) in soil directly was evaluated at Los Alamos for use in the remediation of contaminated sites (Radziemski and Cremers, 1990).

Some research focused on diagnostics and enhancements. The plasma generates shock waves that can be heard and recorded as acoustic signals, whose strengths are related to the energy deposited in the medium. The acoustic properties of the spark were first studied by Belyaev *et al.* (1982). Kitamori *et al.* (1988) started an interesting line of research in particle counting in liquids by using the acoustic effect produced by the plasma. He also made observations of the optical emission. Beginning with the early 1990s, more quantitative uses of acoustic signals were reported, for example by Diaci and Mozina

10 Handbook of Laser-Induced Breakdown Spectroscopy



Figure 1.5 A long spark created by using a cylindrical lens on a filter set on a rotating stage. (Reprinted with permission from Cremers and Radziemski, 1985).

(1992), who studied the blast waveforms detected simultaneously by a microphone and a laser probe. Starting in 1988, there were several reports of attempts to enhance the plasma by the use of auxiliary magnetic or electric fields.

Much interest was shown in the initiation of the spark on single microspheres or droplets. Results included a paper by Chylek *et al.* (1986), on the effect of size and material of liquid spherical particles on laser-induced breakdown. This line of research was continued in a paper by Biswas *et al.* (1988) detailing the irradiance and laser wavelength dependence of plasma spectra from single levitated aerosol droplets. Chang *et al.* (1988) discussed laser-induced breakdown in large transparent water droplets.

In the late 1980s, interest increased in making LIBS more quantitative by addressing factors such as differential excitation. These included many works from the Niemax group in Dortmund, such as Ko *et al.* (1989) and Leis *et al.* (1989). In the former study, the stability of internal standardization was investigated. They found that the chromium to iron intensities in binary mixtures were not a function of time after plasma initiation, hence temperature, or completeness of vaporization. This was in contrast to zinc to copper ratios in brass. The conclusion was that internal standardization was not a given in all cases, but the conditions for its use needed to be established for each situation. In the latter study, the atomization and propagation properties of the plasma plume were investigated.

Studies of toxic and superconducting materials were made. These included analysis of beryllium in beryllium–copper alloys (Millard *et al.*, 1986) and detection of cadmium, lead, and zinc (Essien *et al.*, 1988). The superconducting materials community published many papers on laser ablation for deposition of superconducting thin films and sometimes addressed the optical emission as a diagnostic technique for process monitoring. A method

of monitoring corrosion in the core regions of nuclear reactors was detailed by Adrain and Koebner (1982), and a working system was described.

At the close of the decade, a book edited by Radziemski and Cremers in 1989, *Laser Induced Plasmas and Applications*, summarized the relevant physics, chemistry, and applications at that time. It contained detailed chapters updating the physics of breakdown (Weyl, Chapter 1) and post-breakdown phenomena (Root Chapter 2), and an updated review of the technique (Radziemski and Cremers, Chapter 7).

1.5 LIBS History 1991–2000

As the field proceeded into the 1990s, applications and fundamental studies developed rapidly. There were several useful reviews during this decade including Radziemski (1994), Song *et al.* (1997), and Rusak *et al.* (1998). Hou and Jones (2000) reviewed several techniques with field capability and presented the advantages and disadvantages of each.

More research groups surfaced in the United States and in other countries. In Australia, Grant *et al.* (1991) provided detection limits for minor components in iron ore. This was done with a view to developing a field-based technique. Later, Chadwick's group in Australia analyzed lignite and produced a commercial instrument for coal analysis (Wallis *et al.*, 2000). Sabsabi and Cielo (Canada) started publishing their work on aluminum alloy targets with papers in 1992 and 1995. Palleschi's group in Pisa, Italy began addressing applications with respect to pollutants as described in papers such as the one by Lazzari *et al.* (1994) on the detection of mercury in air.

The application of LIBS to remote analysis began in the 1980s and developed rapidly in the 1990s. It was an important area of investigation by Cremers' group at Los Alamos. Cremers *et al.* (1995) discussed remote elemental analysis by LIBS using a fiber-optic cable. Angel's group also published on the use of a fiber-optic probe to determine lead in paint (Marquardt *et al.*, 1996). LIBS for the analysis of lunar surfaces was first mentioned in papers by Kane *et al.* (1992) and Blacic *et al.* (1992). This was followed by a seminal paper by Knight *et al.* (2000) on the characterization of LIBS for planetary exploration, and a report on the use of LIBS on a prototype Martian Rover (Wiens *et al.*, 2002). Figure 1.6 shows the rover with a prototype LIBS sensor unit on the mast undergoing preliminary testing in the Nevada desert. Also shown is the LIBS sensor unit that was mounted on the mast and a representative spectrum recorded during the testing. The sampling head (~0.9 kg) housed the laser and adjustable focusing and light collection optics. The detection system, a small grating spectrograph, and an ICCD detector were located in the main rover body and were connected to the sampling head by power/control cables and fiber optics.

Efforts to make LIBS more quantitative continued. Davies *et al.* (1996) reported on relevant factors for *in situ* analytical spectroscopy in the nuclear industry. Russo's group at Lawrence Berkeley Laboratory undertook detailed studies of the ablation process as reported by Mao *et al.* (1995). Winefordner's group at the University of Florida initiated studies of the variables influencing the precision of LIBS measurements. Their first publication in this area was by Castle *et al.* (1998), in which a variety of factors were

12 Handbook of Laser-Induced Breakdown Spectroscopy

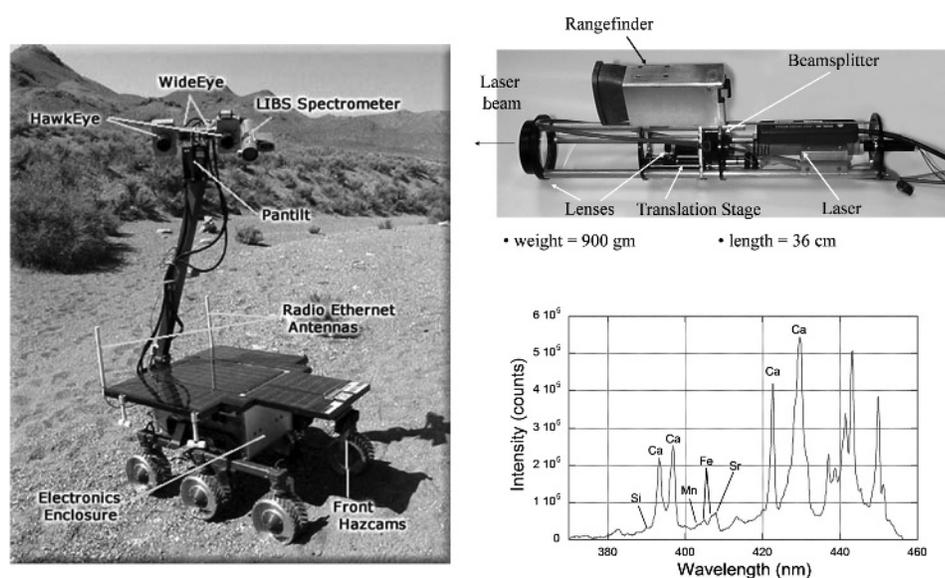


Figure 1.6 The K9 rover in the field (Nevada, USA) with the LIBS sensor mounted on the right side of the mast head instrument suite, circa 2000 (Photo courtesy of NASA Ames Research Center). Also shown are the LIBS mast head instrument and a representative spectrum recorded in the field.

considered and inter- and intra-shot measurement precisions were calculated. The best precision obtained was 0.03%. Gornushkin *et al.* (1999) reported on a curve of growth methodology applied to laser-induced plasma emission spectroscopy. A procedure called “calibration free LIBS” was developed by Palleschi’s group, as explained in a paper by Ciucci *et al.* (1999). In effect, one assumes thermodynamic equilibrium and uses spectral lines representing the bulk of the vaporized material to deduce the concentration of the element of interest. Matrix effects continued to be studied. For example, the effects of water content and grain size were reported by Wisbrun *et al.* (1994). These works and others have sharpened the focus on factors that can enhance or hinder the ability to obtain quantitative results.

Throughout the decade, unique applications continued to emerge. Harith *et al.* (1990) studied the hydrodynamic evolution of laser-driven diverging shock waves. Quantitative simultaneous elemental determinations in alloys, using LIBS in an ultra-high-vacuum, were reported by Thiem *et al.* (1994). The U.S. Army Aberdeen Proving Ground laboratory under Miziolek began its investigations of LIBS with two publications by Simeonsson and Miziolek in 1993 and 1994. They studied LIBS in carbon monoxide, carbon dioxide, methanol, and chloroform and used a variety of laser wavelengths from 193 to 1064 nm. The group of Aragon *et al.* (1993) applied LIBS for determining the carbon content in molten steel. Poulain and Alexander (1995) used LIBS to measure the salt concentration in seawater aerosol droplets. Singh’s group published on the quantification of metal hydrides (Singh *et al.*, 1996) and LIBS spectra from a coal-fired MHD facility (Zhang *et al.*, 1995).

Art analysis has received much attention, for example, as described by Anglos *et al.* (1997), who worked on the diagnostics of painted artworks using LIBS for pigment identification, and Georgiou *et al.* (1998), who described excimer laser restoration of painted artworks. Vadillo and Laserna (1997) published work on depth-resolved analysis of multi-layered samples, a technique that is used in forensic archeometry. Applications to biological materials were developed. Samek *et al.* (1999) studied trace metal accumulation in teeth. Pallikaris *et al.* (1998) reported on the use of LIBS for monitoring corneal hydration while Sattmann *et al.* (1998) started work on polymer identification that resulted in an apparatus to sort plastics.

Determination of the composition of soils and contaminants received considerable attention. Eppler *et al.* (1996) reported on matrix effects in the detection of Pb and Ba in soil. Detection limits of 57 and 42 ppm (w/w) for Pb and Ba, respectively, were achieved. A cylindrical focusing lens yielded higher experimental precision than a spherical lens. Miles and Cortes (1998) performed subsurface heavy-metal detection with the use of a cone penetrometer system. A real-time fiber-optic (FO) LIBS probe for the *in situ* detection of metals in soils was used by Theriault *et al.* (1998).

Much work was directed to improvement in instrumentation and techniques. Undoubtedly the greatest impact was achieved by the introduction of the compact echelle spectrometer mated with ever-more capable CCD detectors, intensified or not. A good introduction to these subjects can be found in Vadillo *et al.* (1996) who reported on space- and time-resolved LIBS using charge-coupled device detection. Also Barnard *et al.* (1993) commented on the design and evaluation of echelle grating optic systems for ICP-OES, and Harnley and Fields (1997) wrote on solid-state array detectors for analytical spectrometry. Bauer *et al.* (1998) described an echelle spectrometer and intensified charge-coupled device combination.

Diode lasers have been proposed as sources because of their small size and simplicity of the operation. An introduction to the subject for laser spectrochemistry was given by Lawrenz and Niemax (1989). A passively Q-switched Nd:YAG microchip laser was described by Zayhowski (2000). The laser was 1 to 2 mm on a side and was diode pumped. Peak powers approaching 0.5 MW were reported. To date, their use has not been widespread.

As lasers with new parameters became available, they were put to use for LIBS applications. The result of using 60 ps Nd:YAG 532 nm pulses was reported by Davis *et al.* (1993). Kagawa *et al.* (1994) wrote on XeCl excimer-laser-induced shock wave plasmas and applications to emission spectrochemical analysis. Sattman *et al.* (1995) discussed the analysis of steel samples using multiple Q-switched Nd:YAG laser pulses. Lasers with pulses of different lengths were used and their results compared. Femtosecond, picosecond, and nanosecond laser ablation of solids was discussed by Chikov *et al.* (1996). Fedosejevs' femtosecond LIBS group has focused on laser pulses of hundreds of microjoules, dubbed "microlibs", as reported by Rieger *et al.* (2000). Microlines imaging was discussed by Mateo *et al.* (2000) of Laserna's group. Angel *et al.* (2001) reported on using dual pulses and pulses of 1.3 ps and 140 fs. Both show very low background signals, so time resolution is not necessary; however, the low signal levels dictate a higher repetition rate and adequate summing of spectra.

Later in the 1990s, the applications turned to very practical problems, such as monitoring environmental contamination, control of material processing, sorting of materials for



Figure 1.7 A portable LIBS surface analyzer, circa 1995. (Reprinted with permission from Yamamoto *et al.* (1996).

recycling, and slurry monitoring. Barrette and Turmel (2000) used LIBS for on-line iron-ore slurry monitoring for real-time process control. Buckley *et al.* (2000) implemented LIBS as a continuous emissions monitor for toxic metals. Palanco and Laserna (2000) studied the full automation of a laser-induced breakdown spectrometer for quality assessment in the steel industry with sample handling, surface preparation, and quantitative analysis capabilities. St-Onge and Sabsabi (2000) published on quantitative depth-profile analysis using LIPS on galvanized coatings on steel. Laser ablation continued as an active area, and was well summarized in a review by Russo *et al.* (2002).

An emphasis on developing rugged, moveable instrumentation emerged at this time. Optical fibers were built into LIBS systems, primarily for carrying the spark light to the spectrometer, but also for the delivery of the laser pulse to the sample as well. More compact echelle spectrographs have been developed. An instrument the size of a small suitcase, used for analysis of contaminants in soils and lead in paint, shown in Figure 1.7 was made in Cremers' Los Alamos lab as reported by Yamamoto *et al.* (1996). Capability, compactness, and portability have improved since that time, as shown in a photo of a more recent field deployable unit in Figure 1.8.

1.6 LIBS History 2001–2012

As we entered the new millennium, new methods of rapidly disseminating LIBS advances appeared. International meetings followed by published proceedings were an important



Figure 1.8 A person-portable LIBS unit for analyzing surfaces. The tip of the probe is placed on the surface and the laser is fired to record a spectrum (ca. 2010).

mechanism. The first international meeting in 2000 was chaired by Palleschi and Tognoni in Pisa, Italy (Corsi *et al.*, 2001). It was followed by international meetings in 2002 in Orlando, Florida, USA, chaired by Miziolek (Hahn *et al.*, 2003), 2004 in Malaga, Spain chaired by Laserna (Laserna and Omenetto, 2005), in 2006 in Montreal, Canada, chaired by Sabsabi (Sabsabi and Russo, 2007), in 2008 in Berlin, Germany, chaired by Panne (Niemax and Panne, 2009), in 2010 in Memphis, Tennessee, USA, chaired by Singh (Singh *et al.*, 2011), and in 2012 in Luxor, Egypt chaired by Harith. In the intermediate years, local meetings were held in the United States (NASLIBS) and by the Eastern Mediterranean Group (EMSLIBS). The published papers from all of these meetings provided excellent summaries of the current status of LIBS at the time.

During this period, five books entirely on LIBS were published: Cremers and Radziemski, 2006, Miziolek *et al.*, 2006, Singh and Thakur, 2007, Ahmed and Awan, 2010, and Noll, 2012. Many reviews also have appeared on general and specialized topics pertaining to LIBS, as noted in Table 1.2 below. These will be useful for those seeking in-depth and up-to-date information about a given subject.

Table 1 in the review by Cremers and Chinni (2009) summarized recent studies of LIBS applications and plasma characteristics. The applications and the number of papers they cite for each provide a guide to the landscape of the hottest recent areas of LIBS research at that time. Table 1.3, an analysis of their Table 1, summarizes these statistics, in the order of decreasing number of citations. The number of LIBS-related publications from the year 1966 to 2010 is shown in Figure 1.9, showing a dramatic increase over the last decade.

New or expanded areas of study include explosive, biological, and chemical threat detection; organic materials; medical applications including dentistry; chemometric, and other statistical methods of data analysis; and detection of lanthanides and actinides (especially uranium and its compounds). Also, several papers have now reported observation of doubly ionized lines. For example, Nagli *et al.* (2011) observed Si(III) and Al(III) and Gaft *et al.* (2011) reported recording B(III) and Fe(III) spectral lines.

16 *Handbook of Laser-Induced Breakdown Spectroscopy***Table 1.2** *Reviews and their focus*

Tognoni <i>et al.</i> (2002)	The authors discuss experimental approaches for quantitative microanalysis with the LIBS technique.
Lee <i>et al.</i> (2004)	This review presents applications of LIBS based on the development of fiber-optic (FO) technology and portable instrumentation.
Noll <i>et al.</i> (2006)	This book chapter reviews industrial applications of LIBS.
Babushok <i>et al.</i> (2006)	A thorough review of double- and multiple-pulse configurations, effects, dependence on laser, pulse delay, and other parameters, and a review of the possible mechanisms.
Fotakis <i>et al.</i> (2007)	Chapter 3 in this book reviews LIBS for cultural heritage applications.
Aragón and Aguilera (2008)	The authors discuss the characterization of LIBS plasmas, including references to new works that report electron densities and plasma temperatures on various samples.
Cleveland and Michel (2008)	This article reviews a near-field laser ablation technique as applied to high-resolution nanoscale surface analysis.
Fantoni <i>et al.</i> (2008)	The authors discuss the details of performing quantitative and qualitative analyses with LIBS, including the ablation process.
Cremers and Chinni (2009)	This work is a comprehensive review of the LIBS technique and its applications.
Hahn and Omenetto (2010)	This is a very comprehensive review of LIBS vis-à-vis plasma diagnostics and plasma-particle interactions, as they bear on LIBS analytical capability.
Fortes and Laserna (2010)	The development of fieldable laser-induced breakdown spectrometer: no limits on the horizon. A review of progress in field-deployable LIBS instrumentation.
Konjević <i>et al.</i> (2010)	Spectroscopic diagnostics of laser-induced plasmas. An overview of spectroscopic diagnostics techniques for low-temperature plasmas is presented with an emphasis on electron number density.
Tognoni <i>et al.</i> (2010)	A review and critique of calibration-free LIBS (CF-LIBS), which includes a summary of applications and a discussion of the simplifying assumptions and the degrees to which they may be met.
Michel (2010)	This review makes the case for improving the results of single-shot LIBS which would open up several new applications.
Singh and Rai (2011)	Reviews the use of the laser for biomedical applications with an emphasis on LIBS. Discusses merits and demerits of LIBS with respect to other techniques.
Hahn and Omenetto (2012)	The second part of this review focuses on instruments and methods and applications to materials analysis and a variety of fields.
Rehse <i>et al.</i> (2012)	Reviews the literature on biomedical applications of LIBS and suggests possible future applications.

Table 1.3 LIBS applications and the number of papers cited by Cremers and Chinni (2009)

Application	Number of papers cited
Metals, alloys, carbon, and steel	32
Plasma characteristics, pressure studies, magnetic effects, parameters, LTE, stoichiometry	21
Explosive, biological, and chemical threat detection	14
Cultural heritage, methods, and specific objects	11
Soil analysis, carbon in soils, contamination	11
Minerals, oil, crystals and gems, ceramics	11
Water and aqueous solutions	10
Organics: alcohols, glucose, DNA, blood	9
Surfaces and films	9
Space: Mars, exoMars, Venus, and other topics	9
Toxic metals in liquids	8
Medical field: dentistry, gallstones, some cancers	8
Chemometric and other statistical analysis methods	8
Coal analysis, flue gas	6
Industrial applications	6
Lanthanide/actinide detection	6
Flame-pyrolysis and gas-phase detection	6
Animal tissues, plants, and woods	5
Aerosol: stand-off LIBS, aerosolized drugs	5
Forensic	5
Paint, glass, and cigarettes	4
Machining and circuits	4
Polymers	4
Food	3
Commercialization of LIBS	3

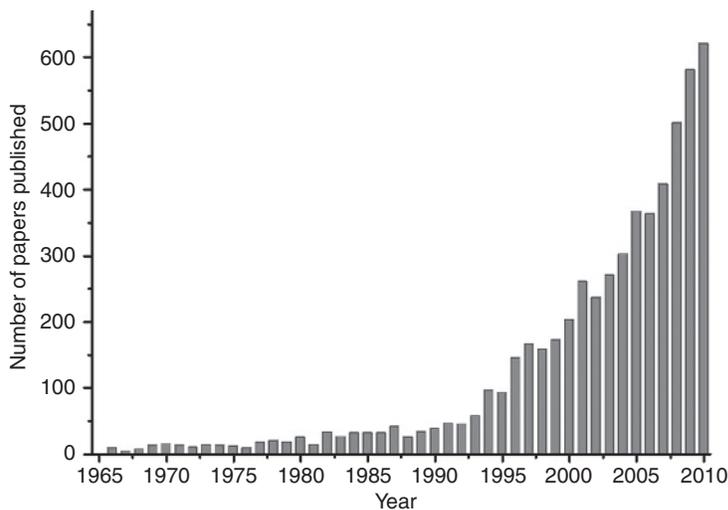


Figure 1.9 LIBS-related papers by year, 1966–2010. In the past 5 years, about 2500 such papers have been published. (Courtesy of Sabsabi, M.).

Table 1.4 Summary of LIBS in different spectral regions

Wavelengths, region	Reference
UV, VUV, down to H(I) 121.6 nm	Jasik <i>et al.</i> (2009)
59–81 nm steel with sulfur	Bengoechea and Kennedy (2004)
VUV down to 150 nm	Radivojevic <i>et al.</i> (2004)
VUV 120–198 nm	Radziemski <i>et al.</i> (2005)
IR to 2000 nm	Radziemski <i>et al.</i> (2007)
IR 2000–4500 nm	Oyebola <i>et al.</i> (2011)
	Yang <i>et al.</i> (2007), (2008)

The wavelength range over which LIBS has been applied is growing as well. Table 1.4 summarizes the extension of LIBS into the VUV and mid-IR over the past decade.

References

- Adrain, R.S. (1982) Some industrial uses of laser induced plasmas. In: *Industrial Applications of Lasers* (ed. H. Koebner), pp. 135–176. New York: John Wiley & Sons, Inc.
- Adrain, R.S. and Watson, J. (1984) Laser microspectral analysis: a review of principles and applications. *Journal of Applied Physics*, 17: 1915–1940.
- Afanas'ev, V. Yu, and Krokhin, O.N. (1967) Vaporization of matter exposed to laser emission. *Soviet Physics Journal of Experimental and Theoretical Physics*, 25: 639–645.
- Ahmed, S.H. and Awan, M.A. (2010). Laser-induced breakdown spectroscopy for Ambient Air Heavy Metals: Development of a Rapid Method for Detection of Heavy Metals in Particulate Matter Using Laser-Induced Breakdown Spectroscopy (LIBS). Saarbrücken, Germany: VDM Verlag Dr. Müller.
- Angel, S.M., Stratis, D.N., Eland, K.L., Lai, T., Berg, M.A., and Gold, D.M. (2001) LIBS using dual- and ultra-short laser pulses. *Fresenius' Journal of Analytical Chemistry*, 369: 320–327.
- Anglos, D., Couris, S., and Fotakis, C. (1997) Artworks: Laser-induced breakdown spectroscopy in pigment identification. *Applied Spectroscopy*, 51: 1025–1030.
- Aragón, C. and Aguilera, J.A. (2008) Characterization of laser-induced plasmas by emission spectroscopy with curve-of-growth measurements. Part II: Effect of the focusing distance and pulse energy. *Spectrochimica Acta Part B*, 63: 793–799.
- Aragon, C., Aguilera, J.A., and Campos, J. (1993) Determination of carbon content in molten steel using laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 47: 606–608.
- Babushok, V.I., DeLucia, F.C., Jr., Gottfried, J.L., Munson, C.A., and Miziolek, A.W. (2006) Double pulse laser ablation and plasma: Laser induced breakdown spectroscopy signal enhancement. *Spectrochimica Acta Part B*, 61: 99–114.
- Barnard, T.W., Crockett, M.J., Ivaldi, J.C., and Lundberg, P.L. (1993) Design and evaluation of an echelle grating optical system for ICP-OES. *Analytical Chemistry*, 65: 1225–1230.
- Barrette, L. and Turmel, S. (2000) On-line iron-ore slurry monitoring for real-time process control of pellet making processes using laser-induced breakdown spectroscopy: graphite vs total carbon detection. *Spectrochimica Acta Part B*, 56: 715–724.

- Bauer, H.E., Leis, F., and Niemax, K. (1998) Laser induced breakdown spectrometry with an echelle spectrometer and intensified charge coupled device detection. *Spectrochimica Acta Part B*, 53: 1815–1825.
- Belyaev, E.B., Godlevskii, A.P., and Kopytin, Y.D. (1978) Laser spectrochemical analysis of aerosols. *Soviet Journal of Quantum Electronics*, 8: 1459–1463.
- Belyaev, E.B., *et al.* (1982) Nature of the acoustic emission during laser breakdown of gaseous disperse systems. *Soviet Technical Physics Letters*, 8: 144–147.
- Bengoechea, J. and Kennedy, E. (2004) Time-integrated, spatially resolved plasma characterization of steel samples in the VUV. *Journal of Analytical Atomic Spectrometry*, 19: 468–473.
- Biberman, L.M. and Norman, G.E. (1967) Continuous spectra of atomic gases and plasma. *Soviet Physics Uspekhi*, 10: 52–54.
- Biswas, A., Latifi, H., Radziemski, L.J., and Armstrong, R.L. (1988) Irradiance and laser wavelength dependence of plasma spectra from single levitated aerosol droplets. *Applied Optics*, 27: 2386–2391.
- Blacic, J.D., Pettit, D.R., and Cremers, D.A. (1992) Laser-induced breakdown spectroscopy for remote elemental analysis of planetary surfaces. Published in the Proceedings of the International Symposium on Spectral Sensing Research, Maui, HI, November 15–20, 1992.
- Brech, F. and Cross, L. (1962) Optical microemission stimulated by a ruby laser. *Applied Spectroscopy*, 16: 59.
- Buckley, S.G., Johnsen, H.A., Hencken, K.K.R., and Hahn, D.W. (2000) Implementation of laser-induced breakdown spectroscopy as a continuous emissions monitor for toxic metals. *Waste Management*, 20: 455–462.
- Buravlev, Yu. M., Nadezhda, B.P., and Babanskaya, L.N. (1974) Use of a laser in spectral analysis of metals and alloys. *Zavodskaya Laoratoriya*, 40: 165–171.
- Buzukov, A.A., Popov, Y.A., and Teslenko, V.S. (1969) Experimental study of explosion caused by focusing monopulse laser radiation in water. *Zhurnal Prikladnoi Mekhaniki i Tekhnicheskoi Fiziki*, 10: 17–22.
- Castle, B.C., Talabardon, K., Smith, B.W., and Winefordner, J.D. (1998) Variables influencing the precision of laser-induced breakdown spectroscopy measurements. *Applied Spectroscopy*, 52: 649–657.
- Cerrai, E. and Trucco, R. (1968) On the matrix effect in laser sampled spectrochemical analysis. *Energia Nucleare*, 15: 581–585.
- Chang, R.K., Eickmans, J.H., Hsieh, W.F., Wood, C.F., Zhang, J.Z., and Zheng, J.B. (1988) Laser-induced breakdown in large transparent water droplets. *Applied Optics*, 27: 2377–2385.
- Chikov, B.N., Momma, C., Nolte, S., von Alvensleben, F., and Tünnerman, A. (1996) Femtosecond, picosecond, and nanosecond laser ablation of solids. *Applied Physics A*, 63: 109–115.
- Chylek, P., Jarzembski, M.A., Chou, N.Y., and Pinnick, R.G. (1986) Effect of size and material of liquid spherical particles on laser-induced breakdown. *Applied Physics Letters*, 49: 1475–1477.
- Ciucci, A., Corsi, M., Palleschi, V., Ratelli, S., Salvetti, A., and Tognoni, E. (1999) New procedure for quantitative elemental analysis by laser-induced plasma spectroscopy. *Applied Spectroscopy*, 53: 960–964.

- Cleveland, D. and Michel, R.G. (2008) A review of near-field laser ablation for high-resolution nanoscale surface analysis. *Applied Spectroscopy Reviews*, 43: 93–110.
- Corsi, M., Palleschi, V., and Tognoni, E. (eds) (2001) Special issue, 1st international conference on laser induced plasma spectroscopy. *Spectrochimica Acta Part B*, 50: 565–1034.
- Cremers, D.A. (1987) The analysis of metals at a distance using laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 41: 572–578.
- Cremers, D.A., Archuleta, F.L., and Martinez, R.J. (1985) Evaluation of the continuous optical discharge for spectrochemical analysis. *Spectrochimica Acta Part B*, 40: 665–679.
- Cremers, D.A., Barefield, J.E., and Koskelo, A.C. (1995) Remote elemental analysis by laser-induced breakdown spectroscopy using a fiberoptic cable. *Applied Spectroscopy*, 49: 857–860.
- Cremers, D.A. and Chinni, R.C. (2009) Laser-induced breakdown spectroscopy – capabilities and limitations. *Applied Spectroscopy Review*, 44: 457–506.
- Cremers, D.A. and Radziemski, L.J. (1983) Detection of chlorine and fluorine in air by laser-induced breakdown spectrometry. *Analytical Chemistry*, 55: 1252–1256.
- Cremers, D.A. and Radziemski, L.J. (1985) Direct detection of beryllium on filters using the laser spark. *Applied Spectroscopy*, 39: 57–60.
- Cremers, D.A. and Radziemski, L.J. (1987) Laser plasmas for chemical analysis. In: *Laser Spectroscopy and its Applications* (eds L.J. Radziemski, R.W. Solarz, J.A. Paisner), pp. 351–415. New York: Marcel Dekker.
- Cremers, D.A. and Radziemski, L.J. (2006) *Handbook of Laser-Induced Breakdown Spectroscopy*. Chichester: John Wiley & Sons, Ltd.
- Cremers, D.A., Radziemski, L.J., and Loree, T.R. (1984) Spectrochemical analysis of liquids using the laser spark. *Applied Spectroscopy*, 38: 721–726.
- Davies, C.M., Telle, H.H., and Williams, A.W. (1996) Remote in situ analytical spectroscopy and its applications in the nuclear industry. *Fresenius' Journal of Analytical Chemistry*, 355: 895–899.
- Davis, L.M., Li, L.Q., and Keefer, D.R. (1993) Picosecond resolved evolution of laser breakdown in gases. *Journal of Physics. D: Applied Physics*, 26: 222–230.
- Debras-Guédon, J. and Liodec, N. (1963) De l'utilisation du faisceau d'un amplificateur a ondes lumineuses par émission induite de rayonnement (laser à rubis), comme source énergétique pour l'excitation des spectres d'émission des éléments. *Comptes-Rendus de l'Académie des Sciences*, 257: 3336–3339.
- Diaci, J. and Mozina, J. (1992) A study of blast waveforms detected simultaneously by a microphone and a laser probe during laser ablation. *Applied Physics A*, 55: 352–358.
- Edwards, A.L. and Fleck, J.A., Jr. (1979) Two-dimensional modeling of aerosol-induced breakdown in air. *Journal of Applied Physics*, 50: 4307–4313.
- Eppler, A.S., Cremers, D.A., Hickmott, D.D., Ferris, M.J., and Koskelo, A.C. (1996) Matrix effects in the detection of Pb and Ba in soils using laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 50: 1175–1181.
- Essien, M., Radziemski, L.J., and Sneddon, J. (1988) Detection of cadmium, lead and zinc in aerosols by laser-induced breakdown spectroscopy. *Journal of Analytical Atomic Spectrometry*, 3: 985–988.
- Evtushenko, T.P., *et al.* (1966) Investigation of air sparks by two synchronized lasers. *Soviet Physics-Technical Physics*, 11: 818–822.

- Fantoni, R., Caneve, L., Colao, F., Fornarini, L., Lazic, V., and Spizzichino, V. (2008) Methodologies for laser-induced breakdown spectroscopy semi-quantitative and quantitative analysis – a review. *Spectrochimica Acta Part B*, 63: 1097–1108.
- Fortes, F.J. and Laserna, J.J. (2010) The development of fieldable laser-induced breakdown spectrometer: No limits on the horizon. *Spectrochimica Acta Part B*, 65: 975–990.
- Fotakis, C., Anglos, D., Zafiropulos, V., Georgiou, S., and Tonari, V. (2007) *Lasers in the Preservation of Cultural Heritage: Principles and Applications*. New York: Taylor & Francis.
- Gaft, M., Nagli, L., Gornushkin, I., and Groisman, Y. (2011) Doubly ionized ion emission in laser-induced breakdown spectroscopy in air. *Analytical and Bioanalytical Chemistry*, 400: 3229–3237.
- Generalov, N.A., Zimakov, V.P., Kozlov, G.I., Masyukov, V.A., and Raiser, Y.P. (1970) Continuous optical discharge. *Journal of Experimental and Theoretical Physics Letters*, 11: 302–306.
- Georgiou, S., Zafiropulos, V., Anglos, D., Balas, C., Tornari, V., and Fotakis, C. (1998) Excimer laser restoration of painted artworks: procedures, mechanisms and effects. *Applied Surface Science*, 129: 738–745.
- Gornushkin, I.B., Anzano, J.M., King, L.A., Smith, B.W., Omenetto, N., and Winefordner, J.D. (1999) Curve of growth methodology applied to laser-induced plasma emission spectroscopy. *Spectrochimica Acta Part B*, 54: 491–503.
- Grant, K.J., Paul, G.L., and O'Neill, J.A. (1991) Quantitative elemental analysis of iron ore by laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 45: 701–705.
- Hahn, D.W. and Omenetto, N. (2010) Laser-induced breakdown spectroscopy (LIBS), Part I. Review of basic diagnostics and plasma-particle interactions: Still challenging issues within the analytical plasma community. *Applied Spectroscopy*, 64: 335A–366A.
- Hahn, D.W. and Omenetto, N. (2012) Laser-induced breakdown spectroscopy (LIBS), Part II. Review of instrumental and methodological approaches to material analysis and applications to different fields. *Applied Spectroscopy*, 66: 347–419.
- Hahn, D.W., Miziolek, A.W., and Palleschi, V. (eds) (2003) Special Issue on LIBS 2002. *Applied Optics*, 42: 5933–6225.
- Harith, M.A., Palleschi, V., Salvetti, A., Singh, D.P., Tropiano, G., and Vaselli, M. (1990) Hydrodynamic evolution of laser driven diverging shock waves. *Laser and Particle Beams*, 8: 247–252.
- Harnley, J.M. and Fields, R.E. (1997) Solid-state array detectors for analytical spectrometry. *Applied Spectroscopy*, 51: 334A–351A.
- Hou, X.D. and Jones, B.T. (2000) Field instrumentation in atomic spectroscopy. *Microchemical Journal*, 66: 115–145.
- Ivanov, Y.V. and Kopytin, Y.D. (1982) Selective interaction of a train of laser pulses with an aerosol medium. *Soviet Journal of Quantum Electronics*, 12: 355–357.
- Jasik, J., Heitz, J., Pedarnig, J., and Veis, P. (2009) Vacuum ultraviolet laser-induced breakdown spectroscopy analysis of polymers. *Spectrochimica Acta Part B*, 64: 1128–1134.
- Kagawa, K., Kawai, K., Tani, M., and Kobayashi, T. (1994) XeCl excimer laser-induced shock wave plasma and its application to emission spectrochemical analysis. *Applied Spectroscopy*, 48: 198–205.

22 *Handbook of Laser-Induced Breakdown Spectroscopy*

- Kane, K.Y., Cremers, D.A., Elphic, R.C., and McKay, D.S. (1992) An in situ technique for elemental analysis of lunar surfaces. Joint Workshop on New Technologies for Lunar Resource Assessment (6 Apr 1992), Santa Fe, NM. NASA-CR-191918.
- Keefer, D.R., Henriksen, B.B., and Braerman, W.F. (1974) Experimental study of a stationary laser-sustained air plasma. *Journal of Applied Physics*, 46: 1080–1083.
- Kitamori, T., Yokose, K., Suzuki, K., Sawada, T., and Gohshi, Y. (1988) Laser breakdown acoustic effect of ultrafine particle in liquids and its application to particle counting. *Japanese Journal of Applied Physics*, 27: L983–L985.
- Knight, A.K., Scherbarth, N.L., Cremers, D.A., and Ferris, M.J. (2000) Characterization of laser-induced breakdown spectroscopy (LIBS) for application to space exploration. *Applied Spectroscopy*, 54: 331–340.
- Ko, J.B., Sdorra, W., and Niemax, K. (1989) On the internal standardization in optical spectrometry of microplasmas produced by laser ablation of solid samples. *Fresenius' Zeitschrift für Analytische Chemie*, 335: 648–651.
- Konjević, N., Ivković, M., and Jovićević, S. (2010) Spectroscopic diagnostics of laser-induced plasmas. *Spectrochimica Acta Part B*, 65: 593–602.
- Laserna, J.J. and Omenetto, N. (eds) (2005) Special issue: Third international conference on laser induced plasma spectroscopy and applications. *Spectrochimica Acta Part B*, 60: 877–878.
- Lauterborn, W. (1972) High-speed photography of laser-induced breakdown in liquids. *Applied Physics Letters*, 21: 27–29.
- Lawrenz, J. and Niemax, K. (1989) A semiconductor diode laser spectrometer for laser spectrochemistry. *Spectrochimica Acta Part B*, 44: 155–164.
- Lazzari, C., de Rosa, M., Rastelli, S., Ciucci, A., Palleschi, V., and Savetti, A. (1994) Detection of mercury in air by time resolved laser-induced breakdown spectroscopy technique. *Laser and Particle Beams*, 12: 525–530.
- Lee, W.B., Wu, J., Lee, Y.I., and Sneddon, J. (2004) Recent applications of laser-induced breakdown spectrometry: a review of material approaches. *Applied Spectroscopy Review*, 39: 27–97.
- Lee, Y.I., Song, K., and Sneddon, J. (1997) Laser induced plasmas for analytical atomic spectroscopy. Ch. 5. In: *Lasers in Analytical Atomic Spectroscopy* (eds J. Sneddon, T.L. Thiem, Y.I. Lee), pp. 197–235. New York: VCH.
- Leis, F., Sdorra, W., Ko, J.B., and Niemax, K. (1989) Basic investigations for laser microanalysis: I. Optical emission spectrometry of laser-produced sample plumes. *Mikrochimica Acta [Wein]*, 11: 185–199.
- Lencioni, D.E. (1973) The effect of dust on 10.6- μm laser-induced air breakdown. *Applied Physics Letters*, 23: 12–14.
- Loree, T.R. and Radziemski, L.J. (1981) Laser-induced breakdown spectroscopy: time-integrated applications. *Plasma Chemistry and Plasma Processing*, 1: 271–280.
- Maker, P.D., Terhune, R.W., and Savage, C.M. (1964) Optical third harmonic generation. Proc. 3rd Int. Conf. Quantum Electron, Paris, Columbia University Press, New York, Vol. 2: 1559.
- Mao, X.L., Shannon, M.A., Fernandez, A.J., and Russo, R.E. (1995) Temperature and emission spatial profiles of laser-induced plasmas during ablation using time-integrated emission spectroscopy. *Applied Spectroscopy*, 49: 1054–1062.

- Marich, K.W., Carr, P.W., Treytl, W.J., and Glick, D. (1970) Effect of matrix material on laser-induced elemental spectral emission. *Analytical Chemistry*, 42: 1775–1779.
- Marquardt, B.J., Goode, S.R., and Angel, S.M. (1996) In situ determination of lead in paint by laser-induced breakdown spectroscopy using a fiber-optic probe. *Analytical Chemistry*, 68: 977–981.
- Mateo, M.P., Palanco, S., Vadillo, J.M., and Laserna, J.J. (2000) Fast atomic mapping of heterogeneous surfaces using microline-imaging laser-induced breakdown spectrometry. *Applied Spectroscopy*, 54: 1429–1434.
- Measures, R.M. and Kwong, H.S. (1979) TABLASER:trace (element) analyzer based on laser ablation and selectively excited radiation. *Applied Optics*, 18: 281–286.
- Michel, A.P.M. (2010) Review: Applications of single-shot laser-induced breakdown spectroscopy. *Spectrochimica Acta Part B*, 65: 185–191.
- Miles, B. and Cortes, J. (1998) Subsurface heavy-metal detection with the use of a laser-induced breakdown spectroscopy (LIBS) penetrometer system. *Field Analytical Chemistry and Technology*, 2: 75–87.
- Millard, J.A., Dalling, R.D., and Radziemski, L.J. (1986) Time resolved laser-induced breakdown spectrometry for the rapid determination of beryllium in beryllium-copper alloys. *Applied Spectroscopy*, 40: 491–494.
- Miziolek, A.W., Palleschi, V., and Schechter, I. (eds) (2006) *Laser-Induced Breakdown Spectroscopy (LIBS), Fundamentals and Applications*. Cambridge: Cambridge University Press.
- Moenke, H. and Moenke-Blankenburg, L. (1973) *Laser Microspectrochemical Analysis*. New York: A. Hilger, London and Crane, Russak and Co., Inc.
- Moenke-Blankenburg, L. (1989) *Laser Micro Analysis*. New York: John Wiley & Sons, Inc.
- Nagli, L., Gaft, M., and Gornushkin, I. (2011) Comparison of single and double-pulse excitation during the earliest stage of laser induced plasma. *Analytical and Bioanalytical Chemistry*, 400: 3207–3216.
- Niemax, K., and Panne, U. (eds) (2009) Special Issue: Fifth international conference on LIBS. *Spectrochimica Acta Part B*, 64: 929.
- Noll, R. (2012) *Laser-Induced Breakdown Spectroscopy*. Berlin: Springer.
- Noll, R., Sturm, V., Stepputat, M., Whitehouse, A., Young, J., and Evans, P. (2006) Industrial applications of LIBS. In: *Laser-Induced Breakdown Spectroscopy (LIBS) Fundamentals and Applications* (eds A.W. Miziolek, V. Palleschi, I. Schechter), pp. 400–439. Cambridge: Cambridge University Press.
- Oyebola, O., Hommerich, U., Brown, E. *et al.* (2011) Concentration dependent studies on the laser-induced mid-infrared emission from KCl-NaCl tablets. *Photonics Letters of Poland*, 3: 171–174.
- Palanco, S. and Laserna, J.J. (2000) Full automation of a laser-induced breakdown spectrometer for quality assessment in the steel industry with sample handling, surface preparation and quantitative analysis capabilities. *Journal of Analytical Atomic Spectrometry*, 15: 1321–1327.
- Pallikaris, I.G., Ginis, H.S., Kounis, G.A., Anglos, D., Papazoglou, T.G., and Naoumidis, L.P. (1998) Corneal hydration monitored by laser-induced breakdown spectroscopy. *Journal of Refractive Surgery*, 14: 655–660.

24 *Handbook of Laser-Induced Breakdown Spectroscopy*

- Piepmeyer, E.H. and Malmstadt, H.V. (1969) Q-switched laser energy absorption in the plume of an aluminium alloy. *Analytical Chemistry*, 41: 700–707.
- Poulain, D.E. and Alexander, D.R. (1995) Influences on concentration measurements of liquid aerosols by laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 49: 569–579.
- Radivojevic, I., Haisch, C., Niessner, R., Florek, S., Becker-Ross, H., and Panne, U. (2004) Microanalysis by laser-induced plasma spectroscopy in the vacuum ultraviolet. *Analytical Chemistry*, 76: 1648–1656.
- Radziemski, L.J. (1994) Review of selected analytical applications of laser plasmas and laser ablation, 1987–1994. *Microchemical Journal*, 50: 218–234.
- Radziemski, L.J. (2002) From LASER to LIBS, the path of technology development. *Spectrochimica Acta Part B*, 57: 1109–1114.
- Radziemski, L.J. and Cremers, D.A. (1989) Spectrochemical analysis using laser plasma excitation. Ch. 7. In: *Laser-Induced Plasmas and Applications* (eds L.J. Radziemski, D.A. Cremers), pp. 303–325. New York: Marcel Dekker.
- Radziemski, L.J. and Cremers, D.A. (eds) (1989) *Laser-Induced Plasmas and Applications*. New York: Marcel Dekker.
- Radziemski, L.J. and Cremers, D.A. (1990) Laser-induced breakdown spectroscopy: principles, applications, and instruments. *Proceedings of SPIE*, 1318: 71–75.
- Radziemski, L.J., Cremers, D.A., Bostian, M., Chinni, R., and Navarro-Northrup, C. (2007) Laser-induced breakdown spectra in the infrared region from 750 to 2000 nm using a cooled InGaAs diode array detector. *Applied Spectroscopy*, 61: 1141–1146.
- Radziemski, L.J., Cremers, D.A., Benelli, K., Khoo, C., and Harris, R. (2005) Use of the vacuum ultraviolet spectral region for LIBS-based Martian geology and exploration. *Spectrochimica Acta Part B*, 60: 237–248.
- Radziemski, L.J., Cremers, D.A., and Loree, T.R. (1983a) Detection of beryllium by laser-induced breakdown spectroscopy. *Spectrochimica Acta Part B*, 38: 349–353.
- Radziemski, L.J. and Loree, T.R. (1981) Laser-induced breakdown spectroscopy: time-resolved spectrochemical applications. *Plasma Chemistry and Plasma Processing*, 1: 281–293.
- Radziemski, L.J., Loree, T.R., Cremers, D.A., and Hoffman, N.M. (1983b) Time-resolved laser-induced breakdown spectrometry of aerosols. *Analytical Chemistry*, 55: 1246–1251.
- Raizer, Y.P. (1966) Breakdown and heating of gases under the influence of a laser beam. *Soviet Physics Uspekhi*, 8: 650–673.
- Raizer, Y.P. (1977) *Laser-Induced Discharge Phenomena*. New York: Consultants Bureau.
- Ready, J.F. (1971) *Effects of High-Power Laser Radiation*. New York: Academic Press.
- Ready, J.F. (2001) *LIA Handbook of Laser Materials Processing*. Orlando, FL: Laser Institute of America.
- Rehse, S.J., Salimnia, H., and Miziolek, A.W. (2012) Laser-induced breakdown spectroscopy (LIBS): an overview of recent progress and future potential for biomedical applications. *Journal of Medical Engineering and Technology*, 6: 77–89.
- Rieger, G.W., Taschuk, M., Tsui, Y.Y., and Fedosejevs, R. (2000) Laser-induced breakdown spectroscopy with low-energy laser pulses. *Proceedings of SPIE*, 4087: 1127–1136.
- Runge, E.F., Minck, R.W., and Bryan, F.R. (1964) Spectrochemical analysis using a pulsed laser source. *Spectrochimica Acta*, 20: 733–735.

- Rusak, D.A., Castle, B.C., Smith, B.W., and Winefordner, J.D. (1998) Recent trends and the future of laser-induced breakdown spectroscopy. *Trends in Analytical Chemistry*, 17: 453–461.
- Russo, R.E., Mao, X., and Mao, S.S. (2002) Physics of laser ablation in microchemical analysis. *Analytical Chemistry*, 74: 70A–77A.
- Sabsabi, M. and Cielo, P. (1992) Laser-induced breakdown spectroscopy on aluminum alloy targets. *SPIE*, 2069: 191–201.
- Sabsabi, M. and Cielo, P. (1995) Quantitative analysis of aluminum alloys by laser-induced breakdown spectroscopy and plasma characterization. *Applied Spectroscopy*, 49: 499–507.
- Sabsabi, M. and Russo, R. (eds) (2007) Special Issue: Fourth international conference on LIBS. *Spectrochimica Acta Part B*, 62: 1285.
- Samek, O., Beddows, D.C.S., Telle, H.H., Morris, G.W., Liska, M., and Kaiser, J. (1999) Quantitative analysis of trace metal accumulation in teeth using laser-induced breakdown spectroscopy. *Applied Physics A*, 69: 179–182.
- Sattman, R., Sturm, V., and Noll, R. (1995) Laser-induced breakdown spectroscopy of steel samples using multiple Q-switch Nd:YAG laser pulses. *Journal of Physics. D: Applied Physics*, 28: 2181–2187.
- Sattmann, R., Moench, I., Krause, H., *et al.* (1998) Laser-induced breakdown spectroscopy for polymer identification. *Applied Spectroscopy*, 52: 456–461.
- Schroeder, W.W., van Niekirk, J.J., Dicks, L., Strasheim, A., and Piepen, H.v.d. (1971) A new electronic time resolution system for direct reading spectrometers and some applications in the diagnosis of spark and laser radiations. *Spectrochimica Acta Part B*, 26: 331–340.
- Scott, R.H. and Strasheim, A. (1970) Laser induced plasmas for analytical spectroscopy. *Spectrochimica Acta Part B*, 25: 311–332.
- Simeonsson, J.B. and Miziolek, A.W. (1993) Time-resolved emission studies of ArF laser produced microplasmas. *Applied Optics*, 32: 939–947.
- Simeonsson, J.B. and Miziolek, A.W. (1994) Spectroscopic studies of laser-produced plasmas formed in CO and CO₂ using 193, 266, 355, 532, and 1064 nm laser radiation. *Applied Physics B*, 59: 1–9.
- Singh, J.P., Almirall, J.R., Sabsabi, M., and Miziolek, A.W. (2011) Special issue: laser-induced breakdown spectroscopy. *Analytical and Bioanalytical Chemistry*, 400: 3191–3192.
- Singh, J.P., and Thakur, S.N. (eds) (2007) *Laser-Induced Breakdown Spectroscopy*. Amsterdam: Elsevier.
- Singh, J.P., Zhang, H., Yueh, F.Y., and Carney, K.P. (1996) Investigation of the effects of atmospheric conditions on the quantification of metal hydrides using laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 50: 764–773.
- Singh, V.K. and Rai, A.K. (2011) Prospects for laser-induced breakdown spectroscopy for biomedical applications: a review. *Lasers in Medical Science*, 26: 673–687.
- Song, K., Lee, Y.I., and Sneddon, J. (1997) Applications of Laser-Induced Breakdown Spectrometry (LIBS). *Applied Spectroscopy Review*, 32: 183–235.
- St-Onge, L. and Sabsabi, M. (2000) Towards quantitative depth-profile analysis using laser-induced plasma spectroscopy: investigation of galvanized coatings on steel. *Spectrochimica Acta Part B*, 55: 299–308.

- Teslenko, V.S. (1977) Investigation of photoacoustic and photohydrodynamic parameters of laser breakdown in liquids. *Soviet Journal of Quantum Electronics*, 7: 981–984.
- Theriault, G.A., Bodensteiner, S., and Lieberman, S.H. (1998) A real-time fiber-optic LIBS probe for the in situ delineation of metals in soils. *Field Analytical Chemistry and Technology*, 2: 117–125.
- Thiem, T.L., Salter, R.H., Gardner, J.A., Lee, Y.I., and Sneddon, J. (1994) Quantitative simultaneous elemental determinations in alloys using LIBS in an ultra-high-vacuum. *Applied Spectroscopy*, 48: 58–64.
- Tognoni, E., Cristoforetti, G., Legnaioli, S., and Palleschi, V. (2010) Calibration-free laser-induced breakdown spectroscopy: State of the art. *Spectrochimica Acta Part B*, 65: 1–14.
- Tognoni, E., Palleschi, V., Corsi, M., and Cristoforetti, G. (2002) Quantitative microanalysis by laser-induced breakdown spectroscopy: a review of the experimental approaches. *Spectrochimica Acta Part B*, 57: 1115–1130.
- Treytl, W.J., Orenberg, J.B., Marich, K.W., Saffir, A.J., and Glick, D. (1972) Detection limits in analysis of metals in biological materials by laser microprobe optical emission spectrometry. *Analytical Chemistry*, 44: 1903–1904.
- Vadillo, J.M. and Laserna, J.J. (1997) Depth-resolved analysis of multilayered samples by laser-induced breakdown spectrometry. *Journal of Analytical Atomic Spectrometry*, 12: 859–862.
- Vadillo, J.M., Milan, M., and Laserna, J.J. (1996) Space and time-resolved laser-induced breakdown spectroscopy using charge-coupled device detection. *Fresenius' Journal of Analytical Chemistry*, 355: 10–15.
- Wachter, J.R. and Cremers, D.A. (1987) Determination of uranium in solution using laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 41: 1042–1048.
- Wallis, F.J., Chadwick, B.L., and Morrison, R.J.S. (2000) Analysis of lignite using laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 54: 1231–1235.
- Wiens, R.C., Arvidson, R.E., Cremers, D.A., *et al.* (2002) Combined remote mineralogical and elemental identification from rovers: Field and laboratory tests using reflectance and laser-induced breakdown spectroscopy. *Journal of Geophysics Research*, 107: 10.1029/2000JE001439.
- Wisbrun, R., Schechter, I., Niessner, R., Schroeder, H., and Kompa, K.L. (1994) Detector for trace elemental analysis of solid environmental samples by laser plasma spectroscopy. *Analytical Chemistry*, 66: 2964–2975.
- Yamamoto, K.Y., Cremers, D.A., Ferris, M.J., and Foster, L.E. (1996) Detection of metals in the environment using a portable laser-induced breakdown spectroscopy instrument. *Applied Spectroscopy*, 50: 222–233.
- Yang, C., Brown, E., Hommerich, U., Trivedi, S., Samuels, A., and Snyder, A. (2007) Mid-Infrared emission from laser-induced breakdown spectroscopy. *Applied Spectroscopy*, 61: 321–326.
- Yang, C., Brown, E., Hommerich, U., Trivedi, S., Samuels, A., and Snyder, A.P. (2008) Mid-Infrared laser-induced breakdown spectroscopy emissions from alkali metal halides. *Applied Spectroscopy*, 62: 714–716.
- Young, M., Hercher, M., and Yu, C.Y. (1966) Some characteristics of laser-induced air sparks. *Journal of Applied Physics*, 37: 4938–4940.

- Zayhowski, J.J. (2000) Passively Q-switched Nd:YAG microchip lasers and applications. *Journal of Alloys and Compounds*, 303: 393–400.
- Zel'dovich, Ya.B. and Raizer, Yu.P. (2002) *Physics of Shock Waves and High-Temperature Hydrodynamic Phenomena* (eds W.D. Hayes, R.F. Probststein). New York: Dover.
- Zhang, H., Singh, J.P., Yueh, F.Y., and Cook, R.L. (1995) Laser-induced breakdown spectra in a coal-fired MHD facility. *Applied Spectroscopy*, 49: 1617–1623.

